




# Dalbavancin

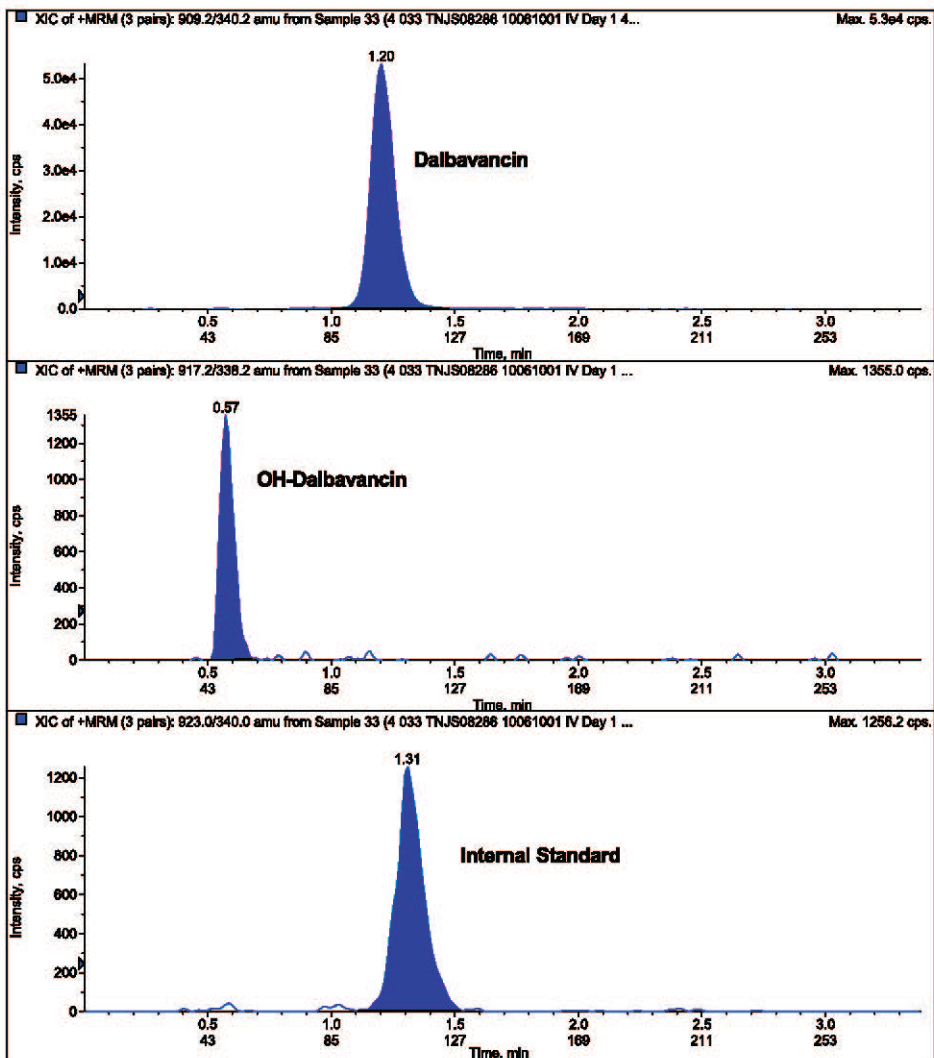

1. Dalbavancin
2. OH-Dalbavancin
3. Internal Standard

Fortis Diphenyl 50x2.1mm 3um

A: 0.1% formic acid in Water

B: 50:50 ACN : MeOH

C: Acetone

0.4ml/min

35oC

MS Detection

Fig. 4. Chromatogram of an incurred urine sample, containing 12.9 µg/mL dalbavancin; x-axis =time [min], y-axis =signal intensity [cps].