

Improving Superficially Porous Particles for Larger Protein Separations



Barry Boyes, Brian Wagner, Ben Libert, Tim Langlois,
Stephanie Schuster, William Miles, Joseph Kirkland

Advanced Materials Technology, Inc.
Wilmington, Delaware, USA
bboyes@advanced-materials-tech.com

Agenda

- Detailed Analysis of Proteins can be HARD
 - High MW polyelectrolytes (peak shape, ESI issues)
 - Little to a lot of heterogeneity (PTMs, chem mods)
 - Subject to change for various environmental reasons
 - Diffusion/mass transfer limitations due to size of molecules
 - Need a combination of methods/approaches
- Recent Enablers in Protein LC/MS
 - Detection Developments: MS Improves!
 - Mobile Phase Developments: Useful Newer Modifiers ←
 - Stationary Phase Developments: Developments in SPP for Proteins ←

Halo Superficially Porous Particles: Fused-Core®

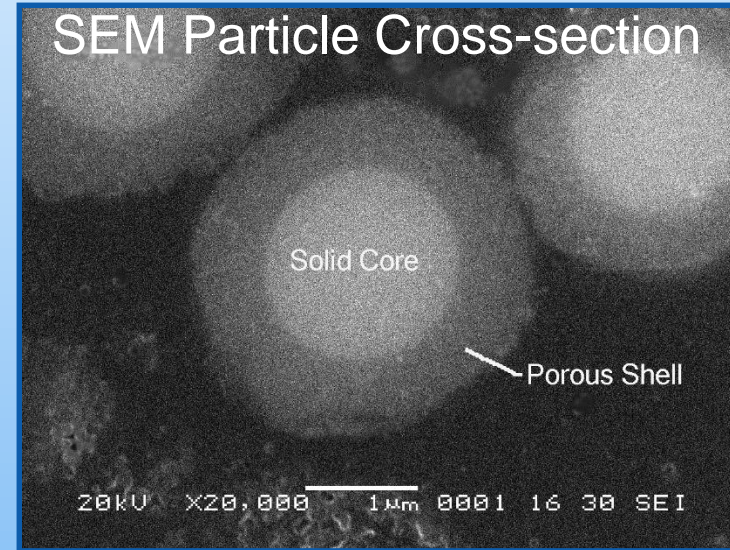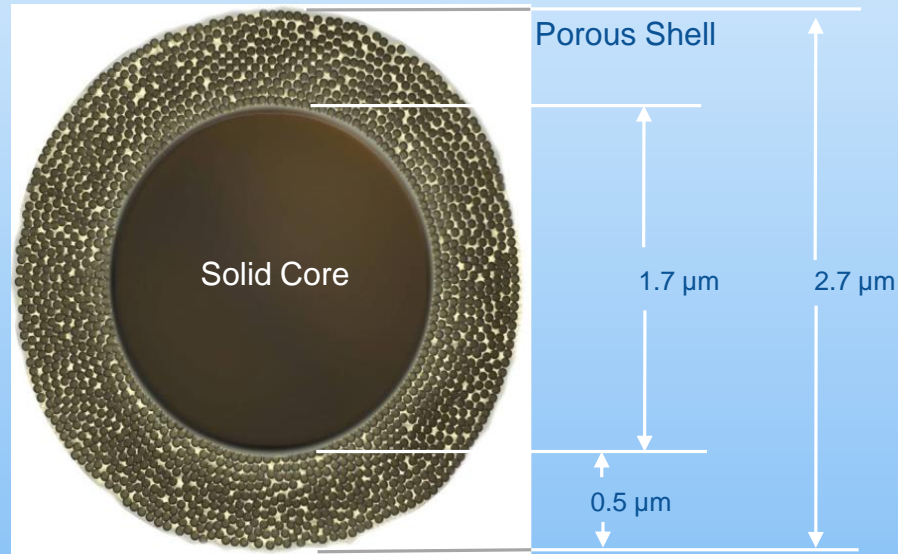

- Low back pressure due to the particle design (solid core with a porous shell)
- No need for specialized HPLC equipment
- Not necessary to filter samples and mobile phase since frits are not as small as needed for sub-2-μm
- High resolution is maintained at high flow rates (flat C-term in van Deemter plot)


Mobile Phases for Protein and Peptide LC/MS

Successful LC/MS depends on Stationary Phase, Mobile Phase and Instrument fitness to task

- TFA is the acidic mobile phase modifier of choice for protein and peptide separations, showing good peak shape and high column efficiency
- Formic acid (and acetic) has been widely adopted for LC/MS applications, with (mostly) reasonable LC performance and excellent MS compatibility
- TFA is widely considered a bad choice for LC/MS, largely due to ESI suppression (low signal), and system persistence after use
- The vast majority of protein LC/MS examples use FA or TFA
- Variants of organic modifier have been reported, but comparatively little drive from current conditions
- Use of elevated temperature (>60°C) is much more common for proteins than in the past – for good reasons!

Improving Retention and Peak Shape Using Ammonium Formate

Column: Halo Peptide ES-C18, 4.6 x 100 mm; Flow rate: 2.0 mL/min; T= 30 C;
 A: Water/acid modifier; B: ACN/0.1% TFA or Formic Acid
 Gradient: 1.5% to 26% B in 15 min.; Injection: 8 µL (800 ng) of synthetic peptides S1-S5

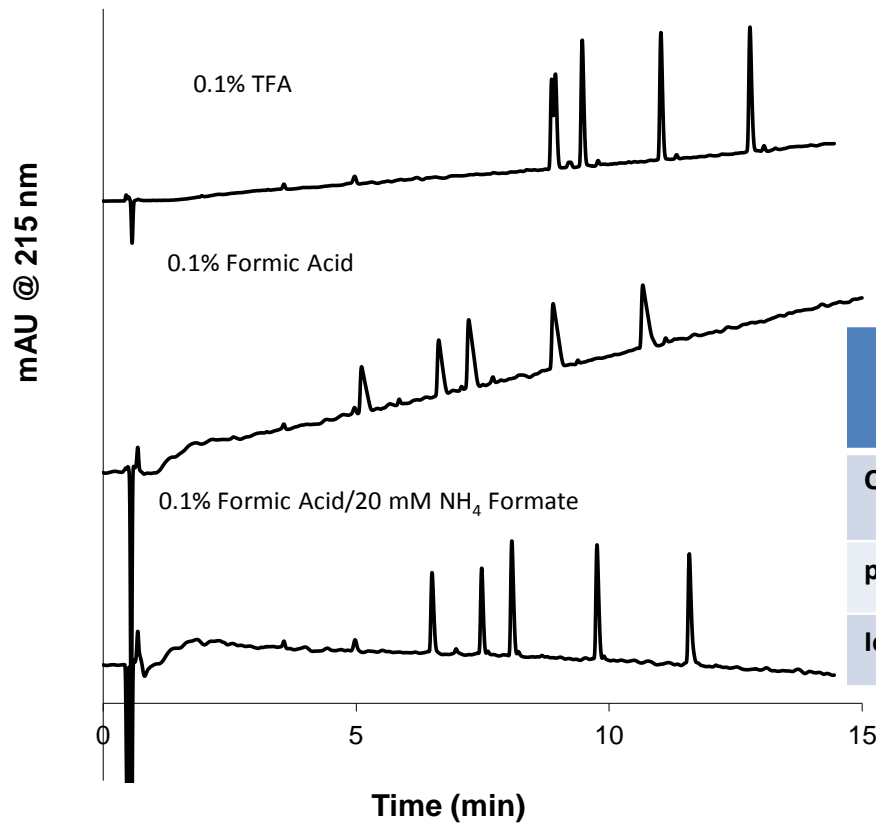

Synthetic Peptide

Retention Standards:


- S1 RGAGGLGLGK-Am
- S2 Ac-RGGGGLGLGK-Am
- S3 Ac-RGAGGLGLGK-Am
- S4 Ac-RGVGGLGLGK-Am
- S5 Ac-RGVVGLGLGK-Am

	TFA 0.1%	Formic Acid 0.1%	Ammonium Formate	AF/FA
Concentration	0.013 M	0.026 M	0.020 M	20 mM AF 26 mM FA
pH	1.8	2.7	c. 7	3.3
Ionic strength	26 mM	4.4 mM	40 mM	c. 44 mM

McCalley, D. V., Effect of buffer on peak shape of peptides in reversed-phase high performance liquid chromatography. *J Chromatogr* **2004**, *1038* (1-2), 77-84.
 Schuster, S. A.; Boyes, B. E.; Wagner, B. M.; Kirkland, J. J., Fast high performance liquid chromatography separations for proteomic applications using Fused-Core® silica particles. *J Chromatogr* **2012**, *1228*, 232-241.

Improved Proteomic Analysis

Column: 0.2 x 150 mm Halo Peptide ES-C18; Flow: 4 μ L/min
 Gradient: 2 - 56% B in 85 min; Pmax - 320 bar;
 A: 0.1% formic acid/10 mM AF/water; B: 80% acetonitrile/A;
 Sample: 5 pmol transferrin, carbonic anhydrase, and apomyoglobin digest mixture
 Detection: Thermo LTQ Ion Trap MS/Michrom ESI interface

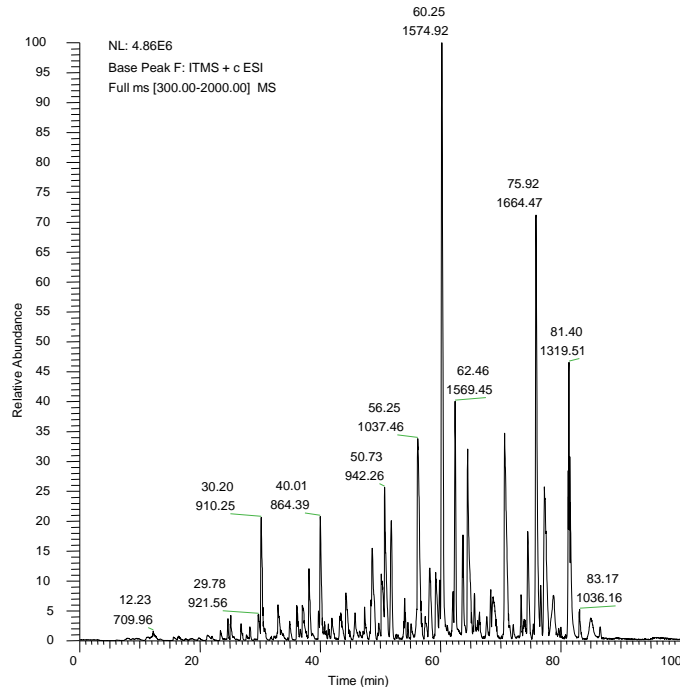

JOHNSON ET AL. / AMMONIUM FORMATE

TABLE 7

Proteomic Results from Canine Prostate Carcinoma Analysis Under Various Chromatographic Conditions for Each Mobile-Phase Modifier

Column length (mm)	Flow rate (μ L/min)	Experiment time (min)	Mobile-phase modifier	Protein IDs ^a	Matched MS/MS spectra	Peptide IDs ^a	Spectra/peptide ID ^b
50	9	21	0.1% FA	44	455	196	2.32
50	9	21	0.1% FA, 10 mM AF	60	697	255	2.73
150	4	140	0.1% FA	70	1142	359	3.18
150	4	140	0.1% FA, 10 mM AF	118	2028	538	3.77

^aResults for each mobile-phase modifier generated from duplicate sample analysis with protein and peptide identifications validated using a 5% false discovery rate.
^bTotal number of database-matched MS/MS spectra, divided by the total number of peptide identifications for each condition from triplicate sample analysis.

TABLE 8

Analysis of the 61 Proteins Commonly Identified Using Both Mobile-Phase Modifier Conditions from LC-MS/MS Analysis Canine Prostate Carcinoma Using a 0.2 \times 150-mm Column

Mobile-phase modifier	Average peptide IDs/protein ^a	Average spectral count/protein ID ^b	Single-spectrum protein IDs ^c
0.1% FA	6.60	20.71	3
0.1% FA, 10 mM AF	9.64	28.56	0

^aThe number of peptides identified from the 61 common identification proteins, divided by the number of common protein identifications.
^bThe total number of database-matched MS/MS spectra from the 61 common identification proteins, divided by total of common protein identifications.
^cProtein identifications from only one single MS/MS spectra after application of a 5% false discovery rate.

Johnson, D.J., Boyes, B.E., Orlando, R.C. The Use of Ammonium Formate as a Mobile-Phase Modifier for LC-MS/MS Analysis of Tryptic Digests. **2013** *J. Biomol. Tech.*, 24, 187-197.

Mobile Phases for Improved Protein LC/MS

-Properties That May Help

Volatility

- Necessary but not sufficient for additives. Must NOT plug our ESI interface and capillary ion entrance path!
- Henry's Law Coefficients (H_{cc}): A higher value of the coefficient indicates ease of transfer of the protonated acid from the idealized aqueous phase of the mobile phase mixture. Not readily available, and not certain to predict partitioning from organic aqueous mixtures.

Low pKa

- Low pH and dissociation of acid; sufficient ionic strength appears beneficial for separation needs, while effect on ESI suppression must be managed

Favor Peptide and Protein Solubility


- Acidic (usually). Fluorinated? Polar? Chaotropic?

Mobile Phases for Improved Protein LC/MS

Properties That May Help

Initial selection and testing indicated some candidates with promise:


Share required features of volatility, lower pKa, but variable protein solubility

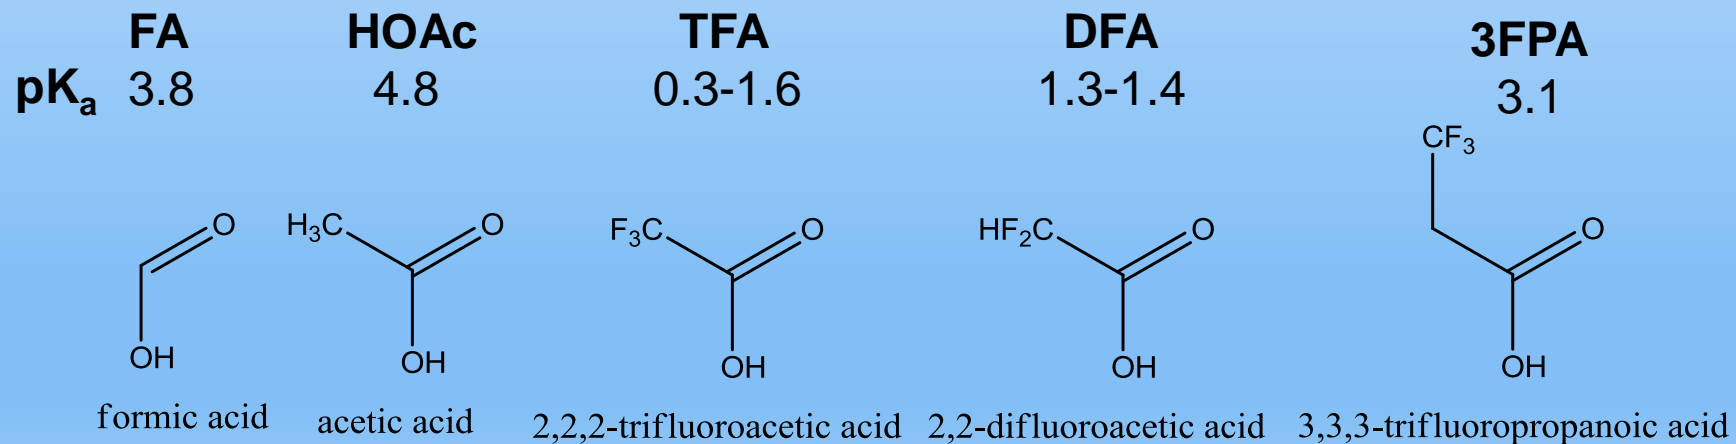

Synthetic Peptide Mixture LC/MS in Several Acidic Modifiers

10 mM Acid; 50pmol 5 peptide mix


2.1 x 150 mm Halo Peptide C18, 0.3mL/min, 2-47%AcN in 40min, 60°C, 300-1800m/z, 4kV, 0.33s

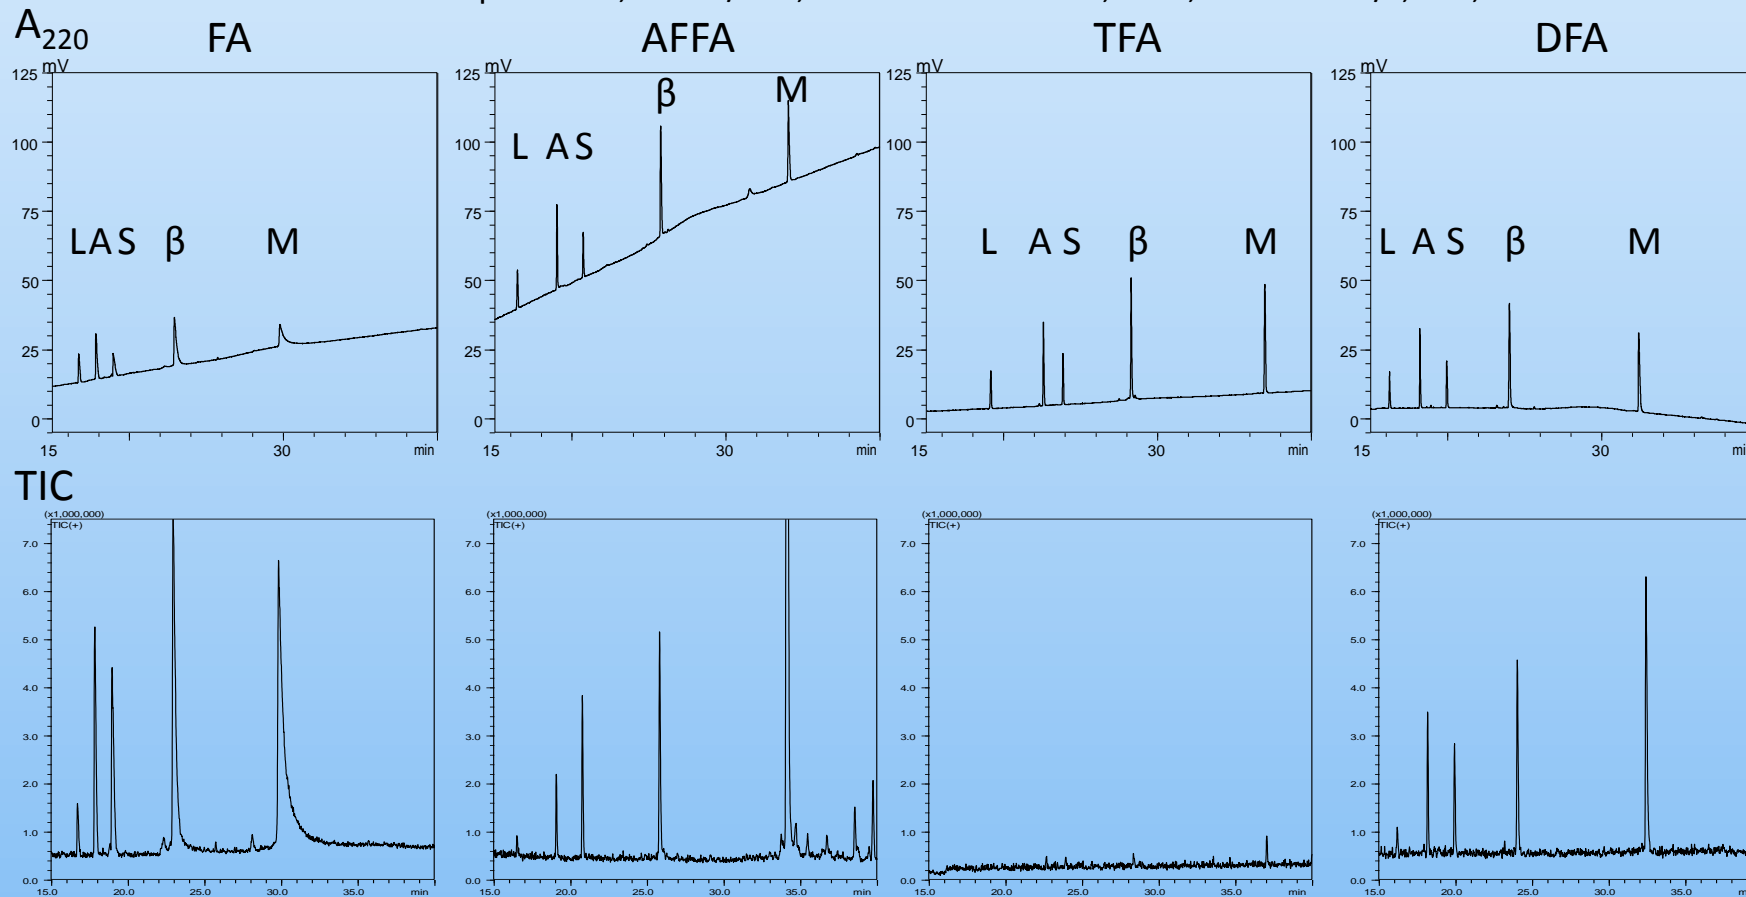


Peptide	Abbrev.	MW
[Leu5]-enkephalin	L	555.6
angiotensin I, human acetate hydrate	A	1297
substance P acetate salt hydrate	S	1348
Melittin, honey bee venom	M	2847
beta-endorphin, human	β	3465

Synthetic Peptide Mixture LC/MS in Several Acidic Modifiers

10 mM acid in mobile phases; 2.1 x 150 mm Halo Peptide C18, 0.3mL/min, 2-47%AcN in 40min, 60°C, 300-1800m/z, 4kV, 0.33s

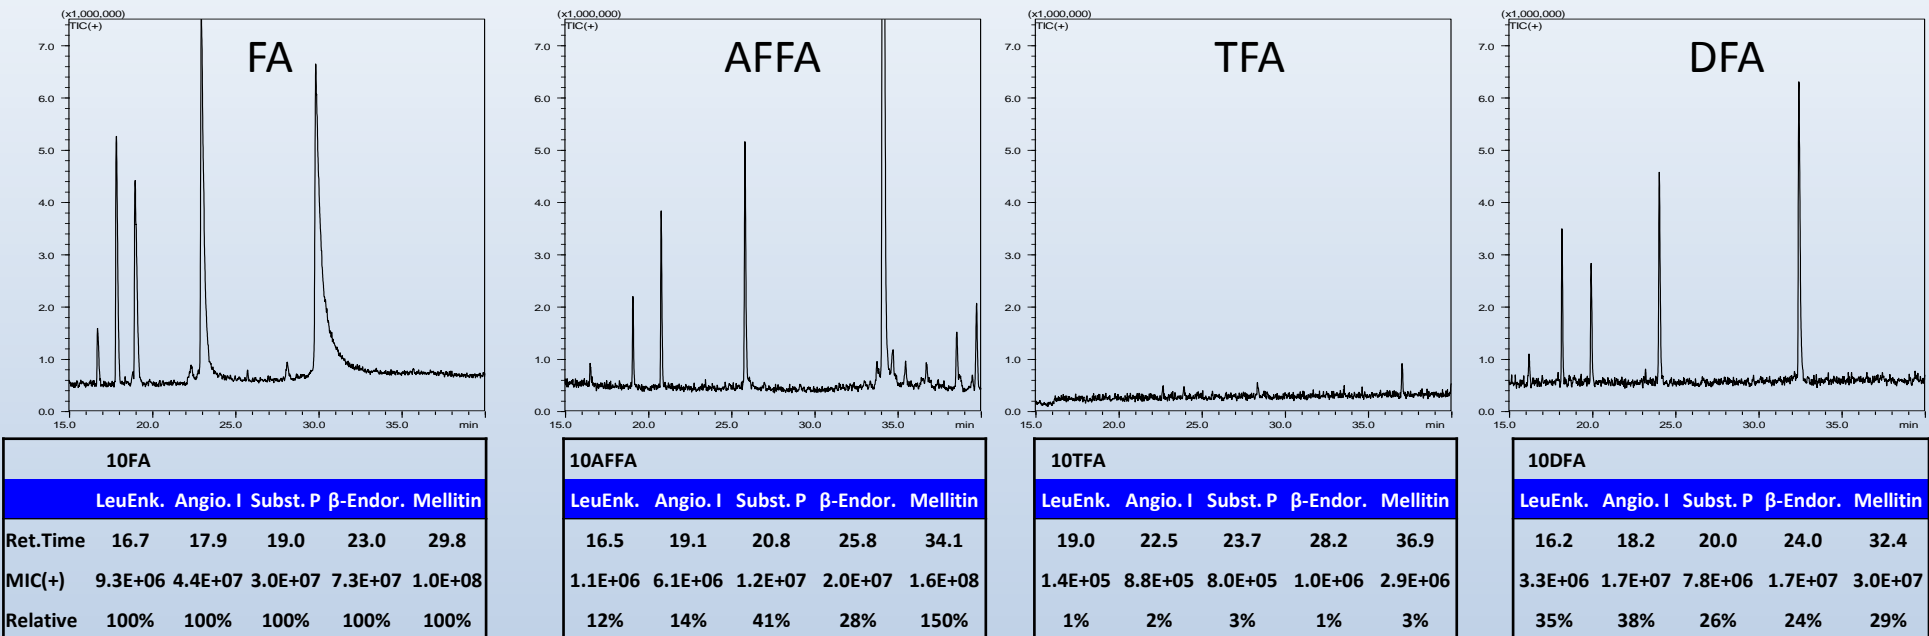

MIC(+) Area Relative to Formic Acid

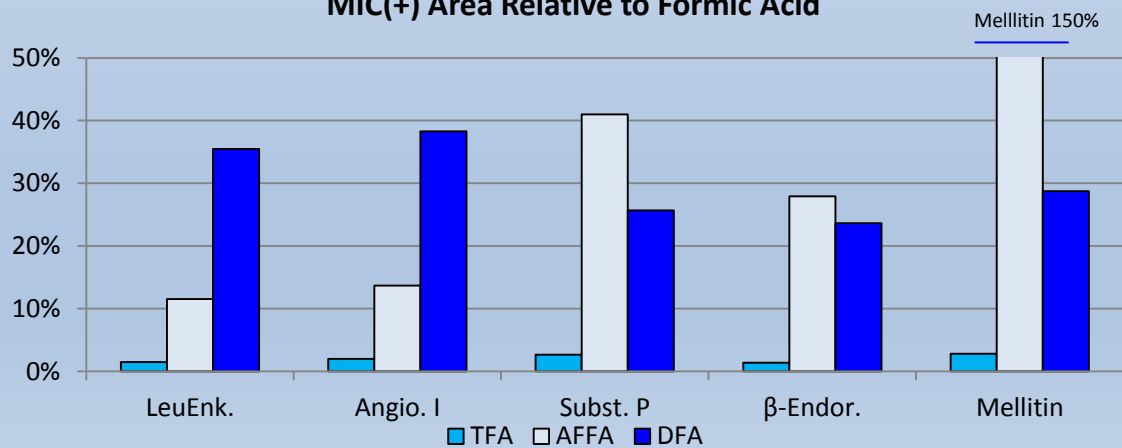

Mean of triplicates for signal intensities at 50 pmol of each peptide. RSD less than 10%.

Summary

- TFA 20-50 fold lower signal
- DFA 3-4 fold lower signal
- FA wider peaks, tailing

Mobile Phases for Improved Protein LC/MS

2.1 x 100 mm
Protein 400 C4

15-55% AcN 30 min

0.35 mL/min; 50°C

25 pmol each protein

R – Ribonuclease

U – rec. Ubiquitin

L – Lysozyme

M – apo-Myoglobin

E – Enolase





Nexera LC system

MS-2020 Single Quad





400 – 2000 m/z 3 pps

3.8 kV ESI





UV (280 nm)

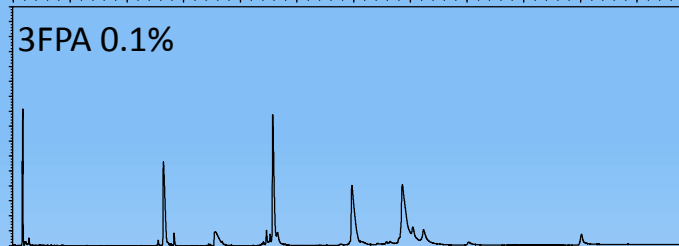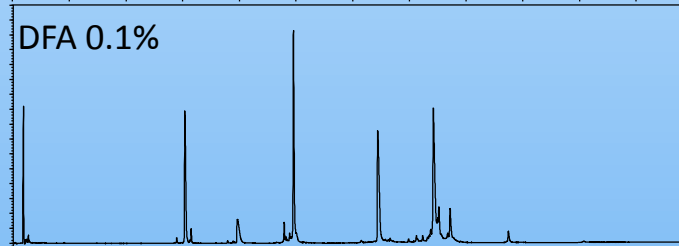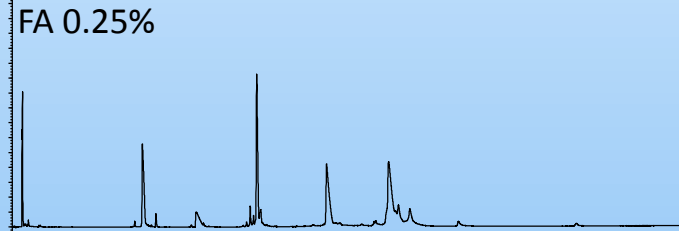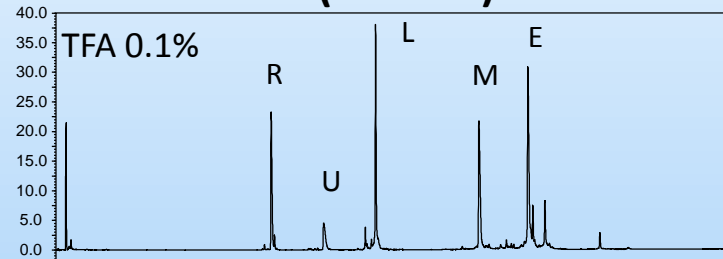

MS (TIC)

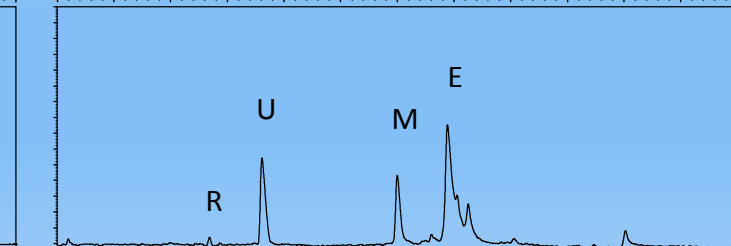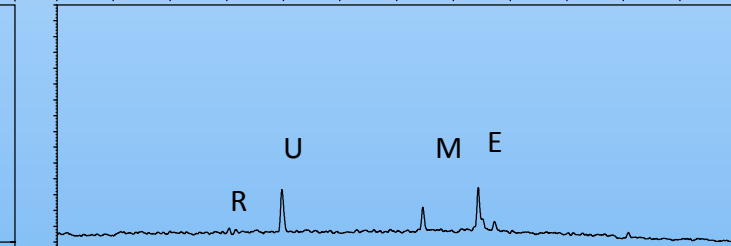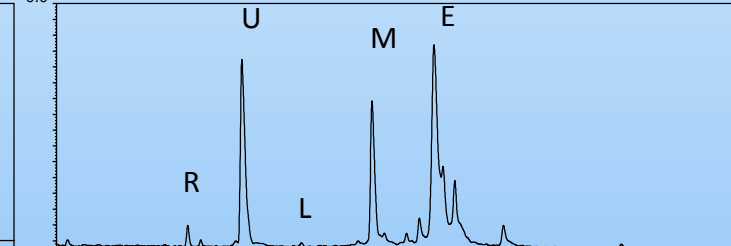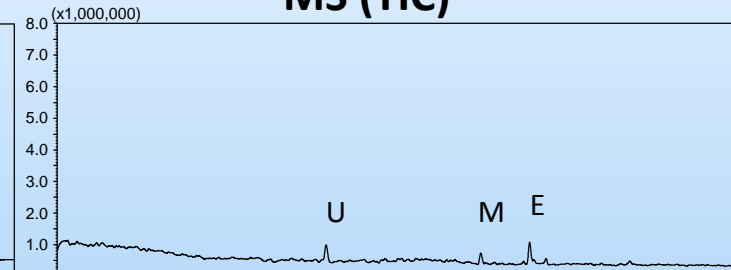

Mobile Phases for Improved Protein LC/MS

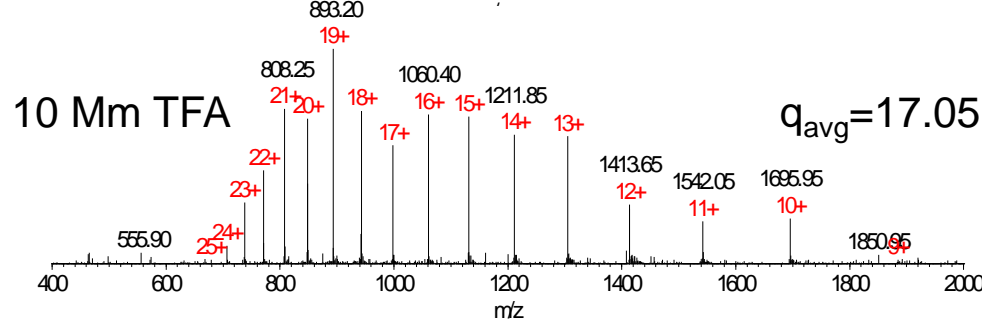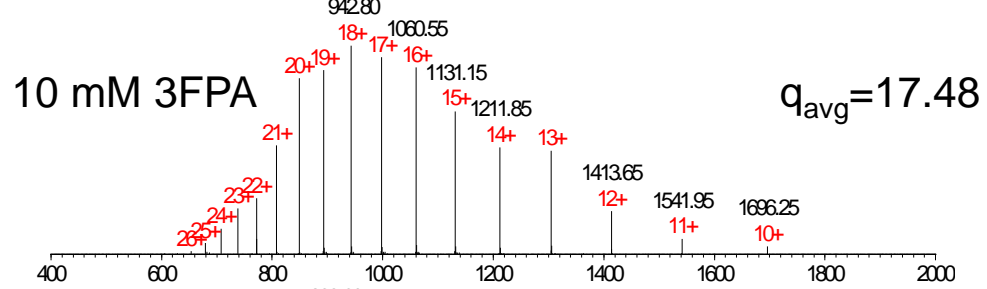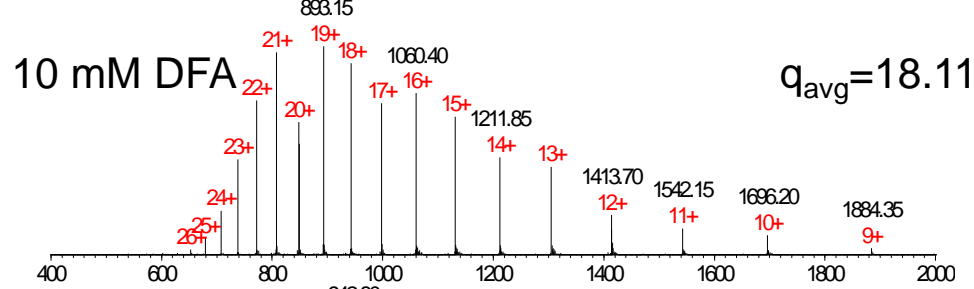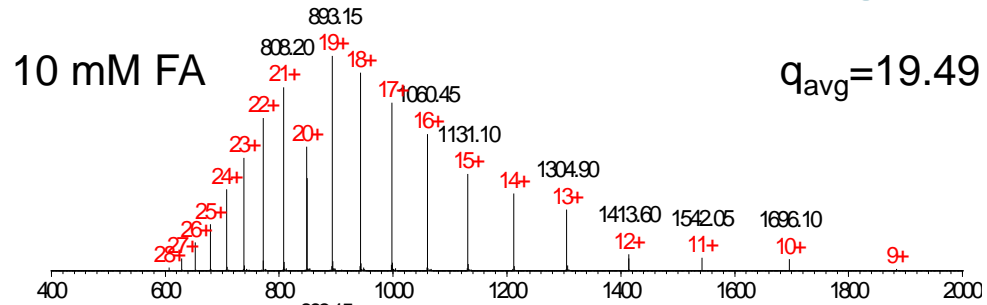


apo-Myoglobin
MS spectra average
ionization state

$$q_{avg} = \frac{\sum_{i=1}^N q_i * w_i}{\sum_{i=1}^N w_i}$$

Subtle changes in charge state


Mobile Phases for Improved Protein LC/MS

- Titration of each acid established suppression of ESI signal as a function of concentration: plateau for FA – 50 mM, others at 10-20 mM
- Graph compares 10 mM of each ion pair reagent to 10 mM FA
- DFA signal 3-5 fold improved, relative to TFA

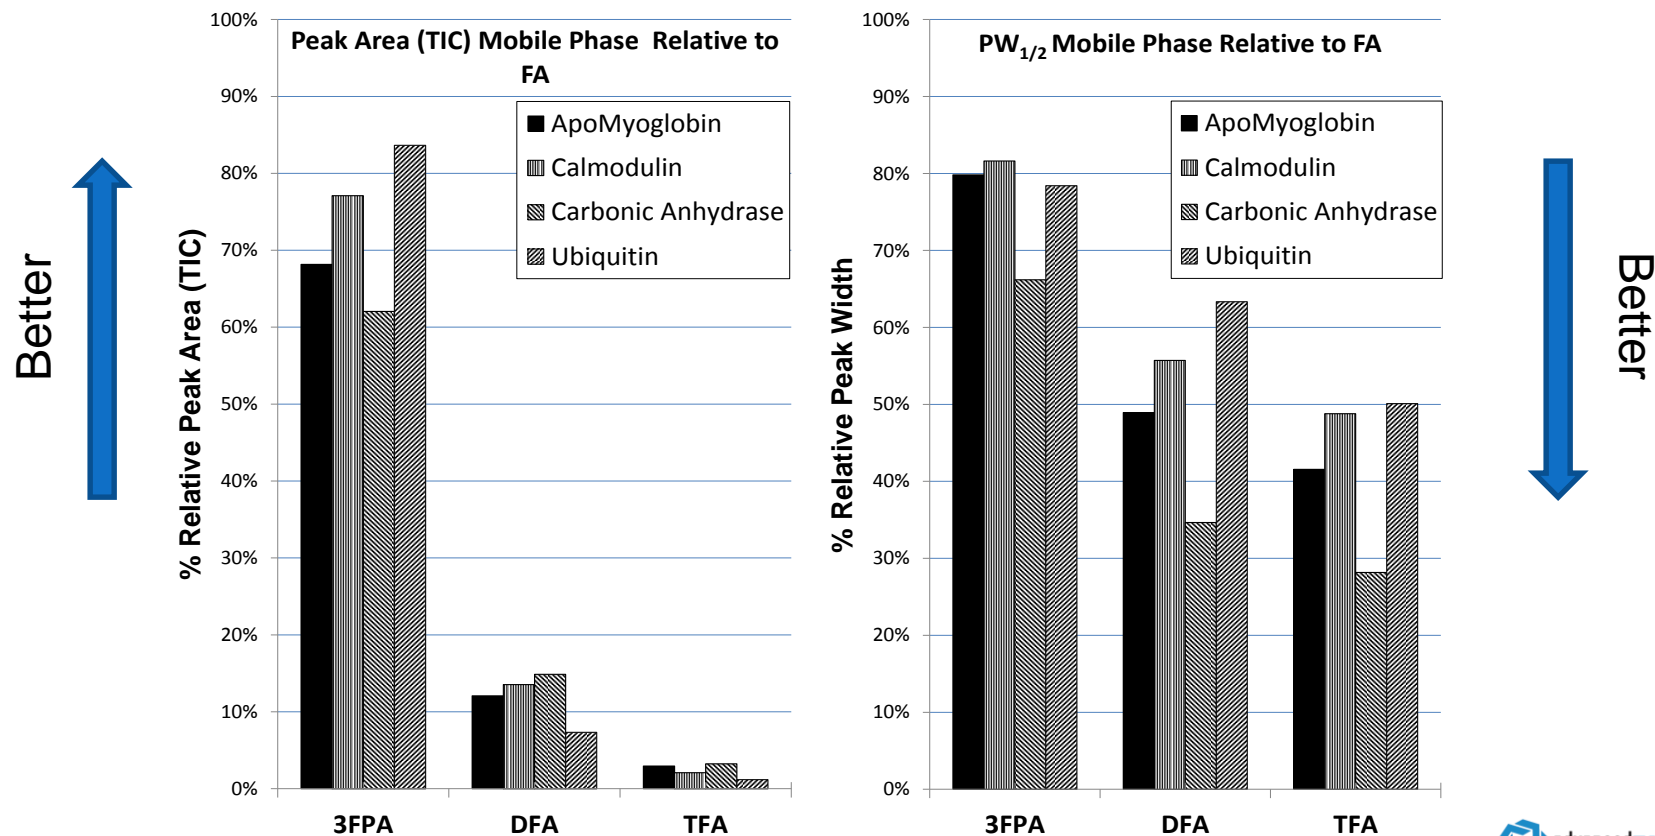

Mobile Phases for Improved mAb LC


2.1 x 150 mm Halo Protein 400 C4; Gradient: 28-38% AcN/0.1% acid as indicated 15 min
Flow: 0.3 mL/min; Temp: 80°C; Sample: 2 μ L of Intact SILu™ Lite SigmaMAb - 0.5 μ g/ μ L (H₂O)

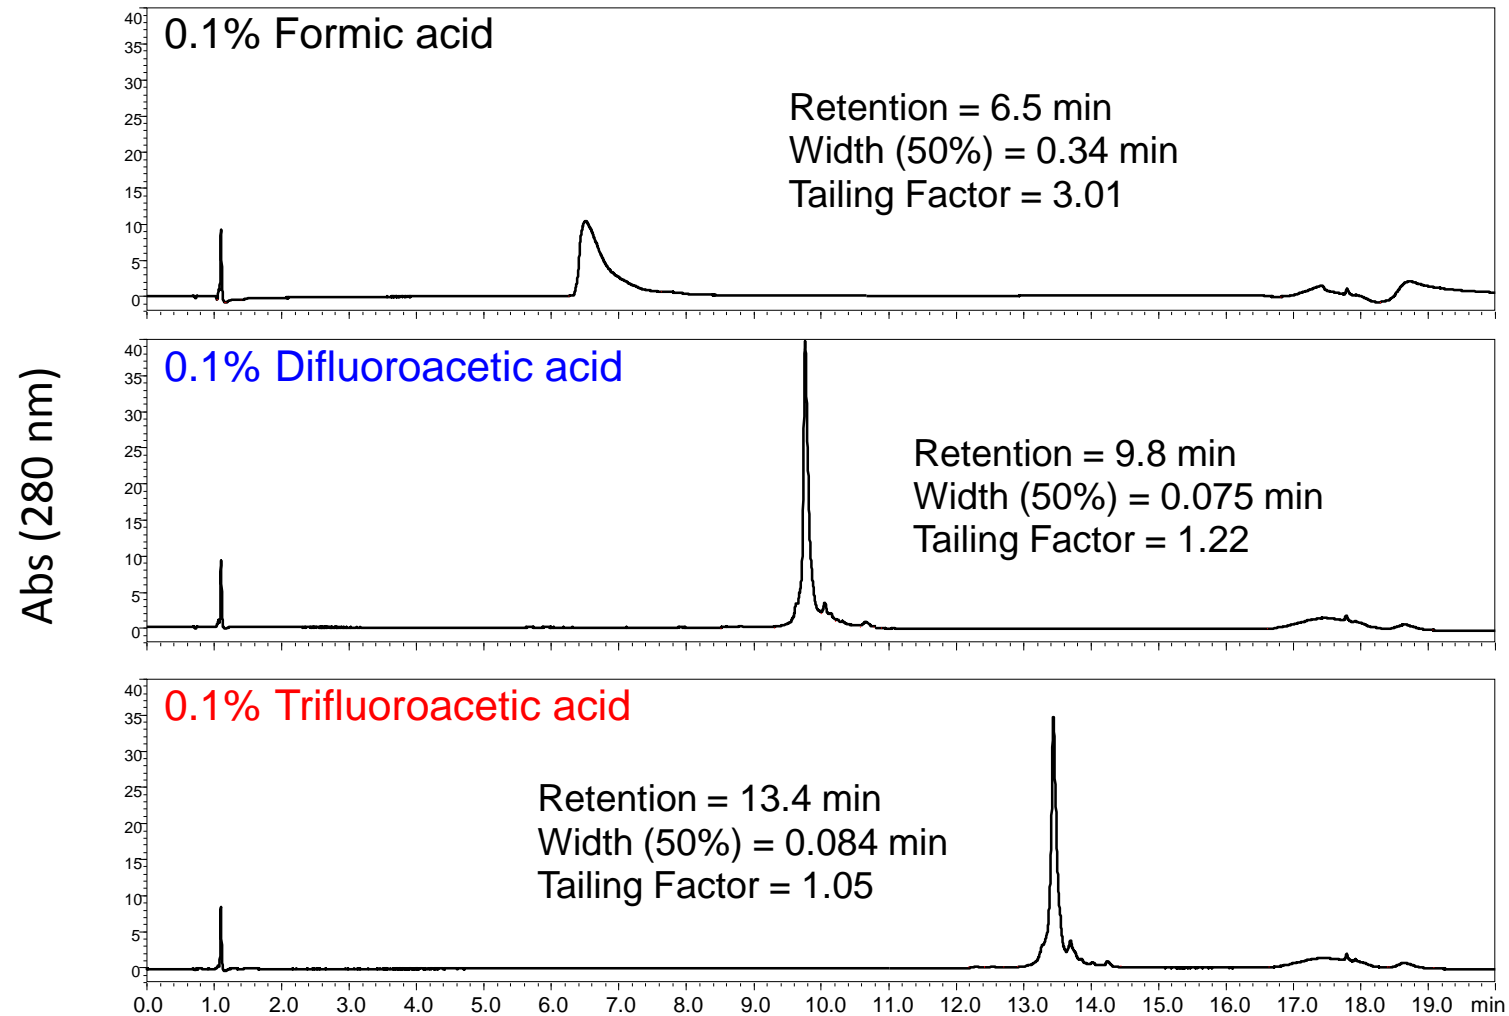


Wide Pore SPP Can Fit the Needs for Protein Science

What is Needed for High Performance Separations of Larger (Bio) Molecules?


- **Pore Size must “fit” molecule size**
 - Restricted diffusion limits efficiency and load capacity
 - Peak capacity effects by kinetic and retention limitations
- **Particle Geometry must Optimize Surface Area/Volume**
 - Shell thickness determines diffusion path and Surface Area
 - Must have “Right” size AND desirable particle distribution
- **Surface Chemistry appropriate to Samples**

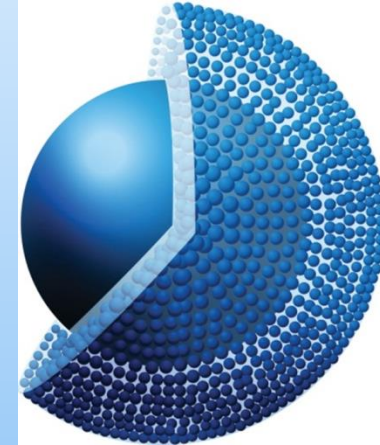

Superficially Porous (Fused-Core[®]) Wide Pore Particles: 160 Å, 400 Å, 1000 Å

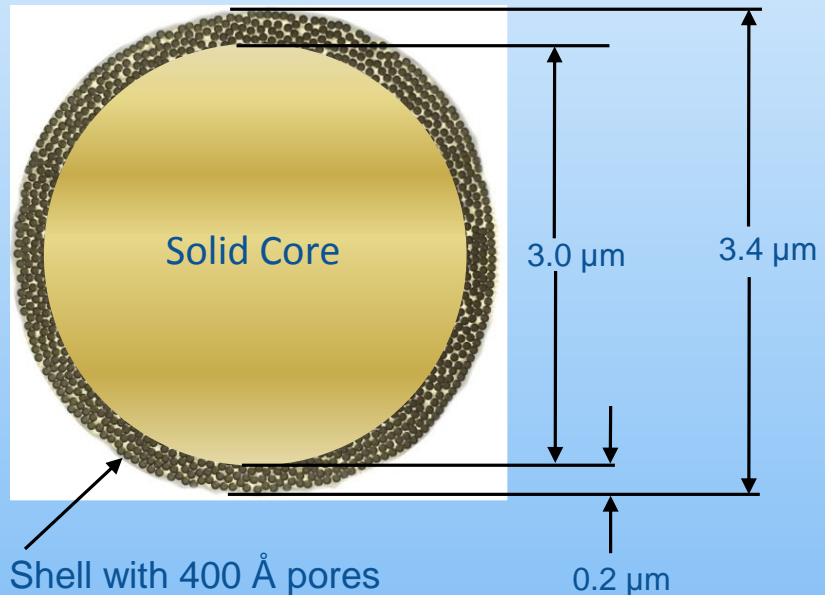

Wide-pore Halo 400 Protein Particles

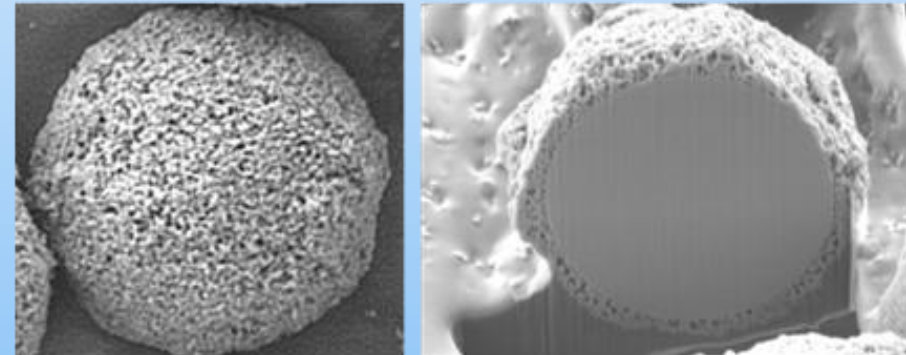


- Example above is 3.4 μm particle/400 Å pore size
- Many variations in shell thickness, pore size and particle size have been studied
- Theory to support “best properties” is complex, with limited tests using proteins, particularly with larger proteins
- Look for compromise in diffusion path for high MW molecules (to maintain small C-term), load tolerance, usability, speed and efficiency

Protein Separation on Wide Pore SPP vs FPP

2.1 mm ID x 150 mm C4 columns
20-50% AcN/0.1% DFA in 24 min
Flow: 0.5 mL/min
Temp: 60°C
1.5 μ L (0.15-0.2 ug each)

1. RNase A 13.7 kDa
2. α -Lactalbumin 14.2 kDa
3. Enolase 93.1 kDa
4. Carbonic Anhydrase 30.0 kDa

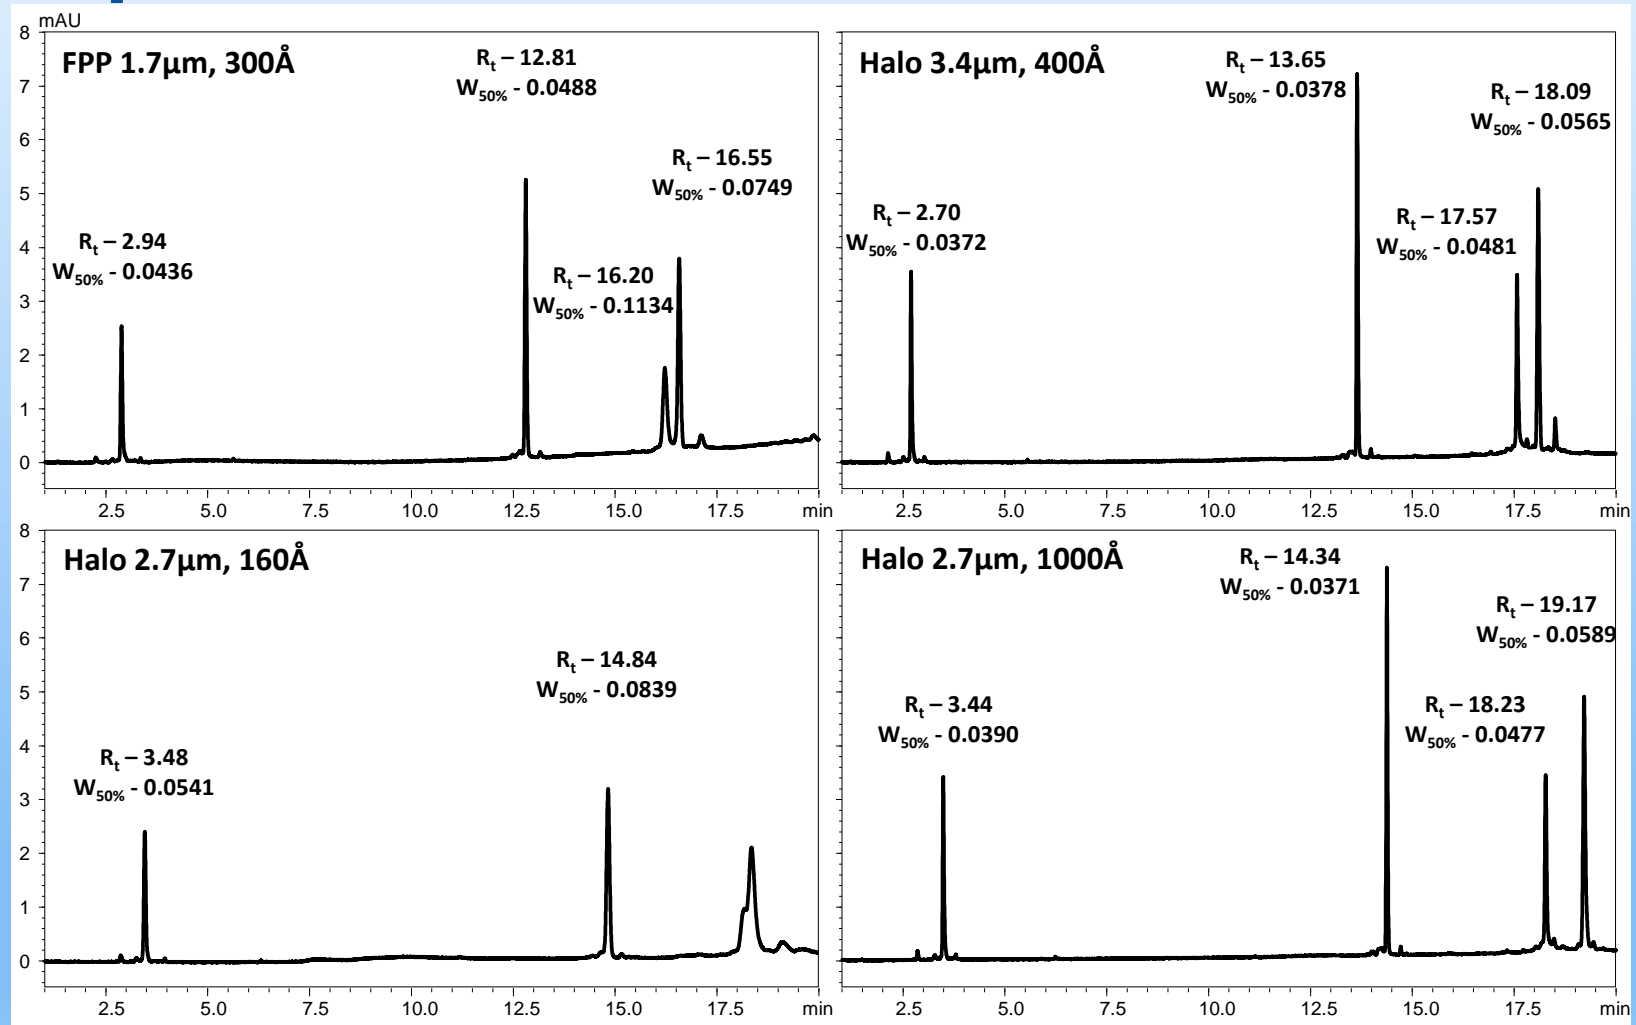


- Improvement in Peak Width and Retention with Larger Pore SPP
- As protein size increases, peak widths decrease with increasing pore size
- Similar results in TFA and DFA as mobile phase acidic modifiers

mAb IgG Separation on Wide Pore SPP vs FPP

High Efficiency Separation of Trastuzumab


Columns: 2.1 x 150 mm; Flow rate: 0.4 mL/min; Mobile Phase A: water/0.1% DFA; Mobile Phase B: acetonitrile/0.1% DFA; Gradient: 27-37% B in 20 min; Injection Volume: 2 μ L (1 μ g); Temp: 80 $^{\circ}$ C

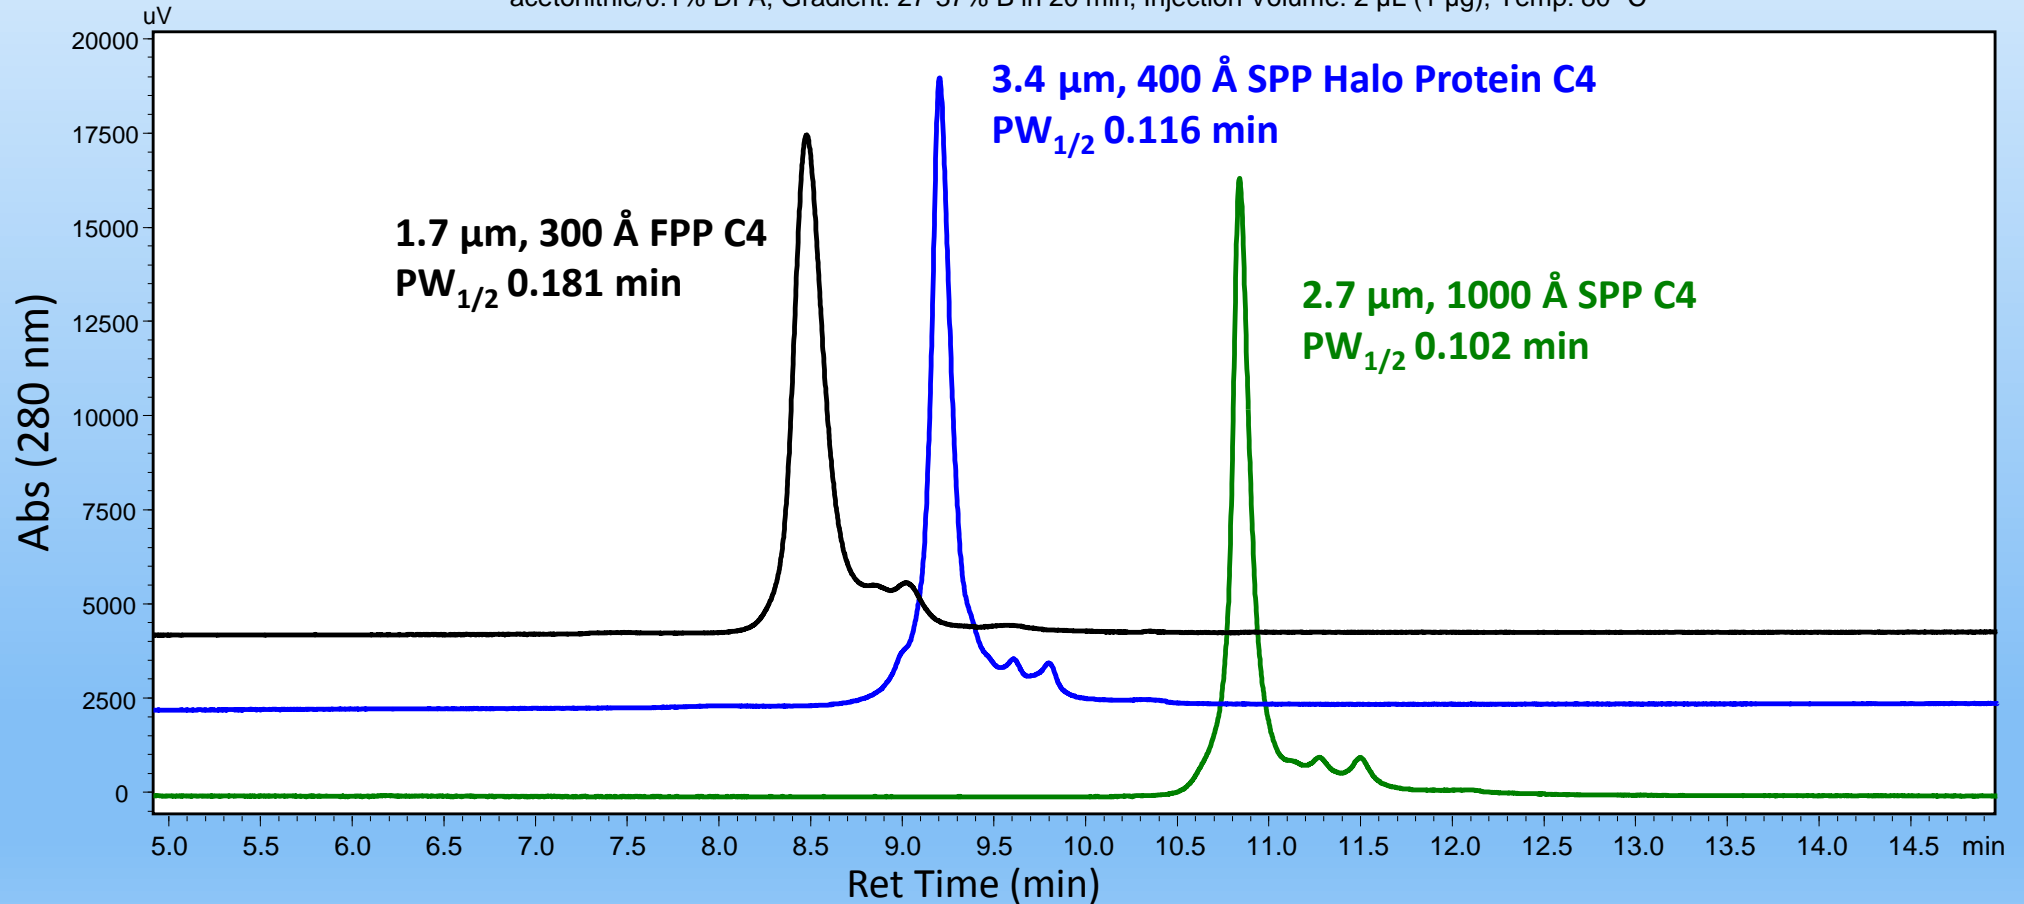

- Large improvement in Peak Width and increased Retention with Larger Pore SPP, moderate additional improvement in Peak Width with Larger Pores

Flow Rate Effects on Peak Volume for mAb IgG


Fixed Volume Gradient Conditions (4.8 mL); Peak Volume = $PW_{1/2} \times \text{Flow Rate}$
Trastuzumab 0.5 μg ; 29-35% AcN in 0.1% DFA; 80°C;

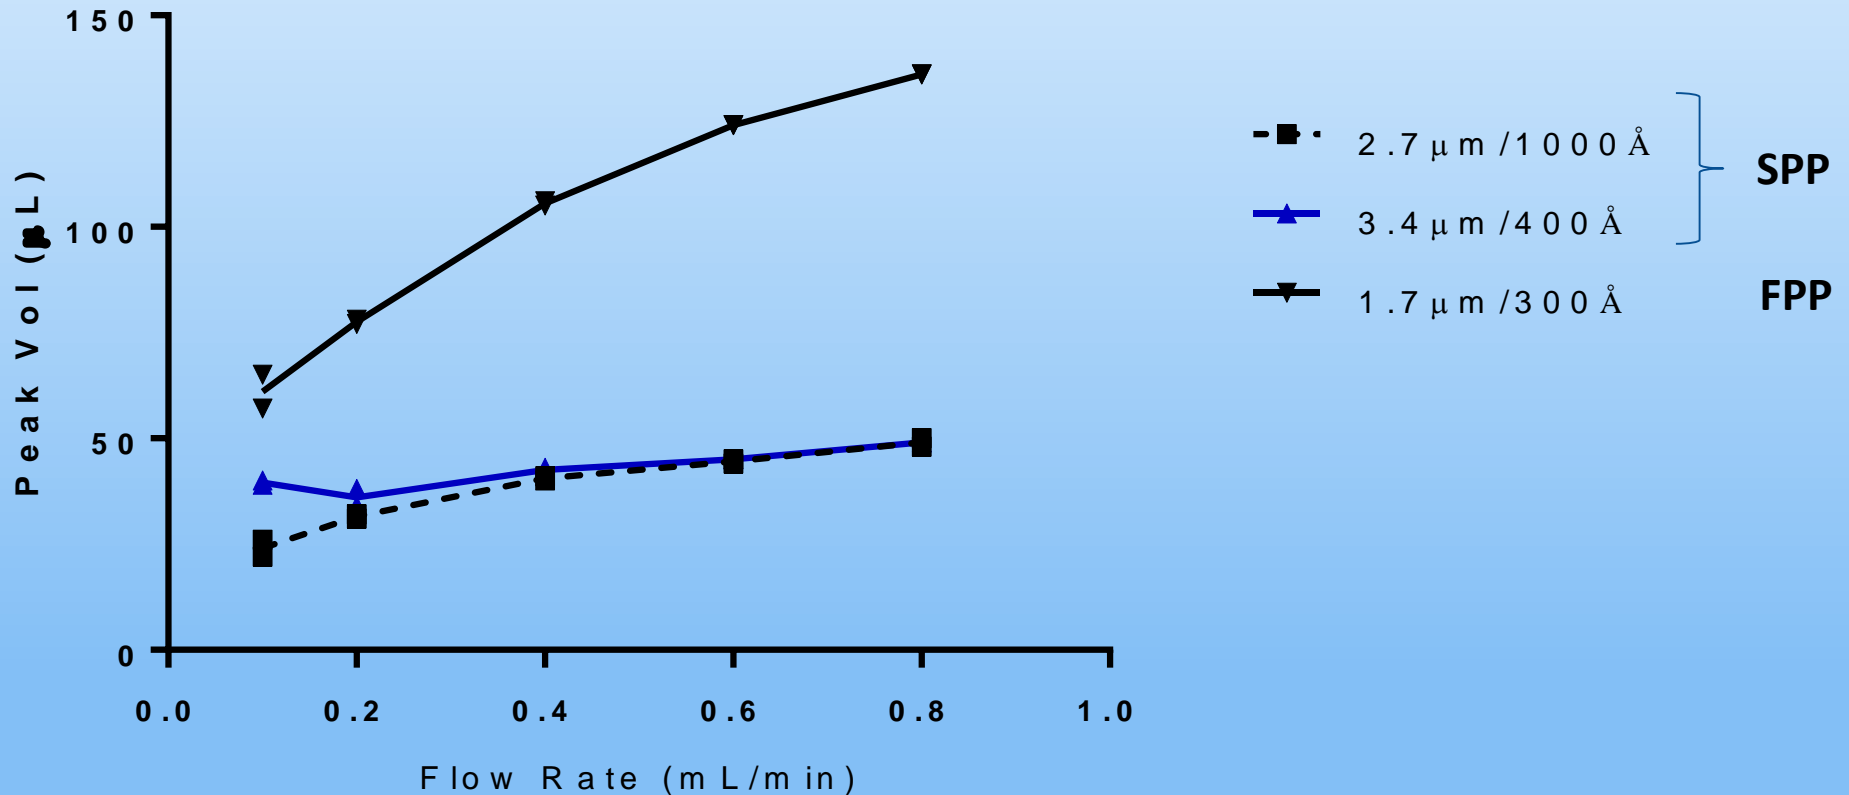

- Mass Transfer is improved for the large pore SPP particles with higher MW protein.
- Trastuzumab and Silumab exhibited similar results
- Retention time matching across columns (gradient shift) exhibited similar results

Load Effects on Peak Width for SPP and FPP for mAb IgG

2.1 mm ID x 150 mm C4 columns; Trastuzumab 0.7 – 140 μg ;
27-37% AcN (0.1% DFA) in 10 min; 80°C

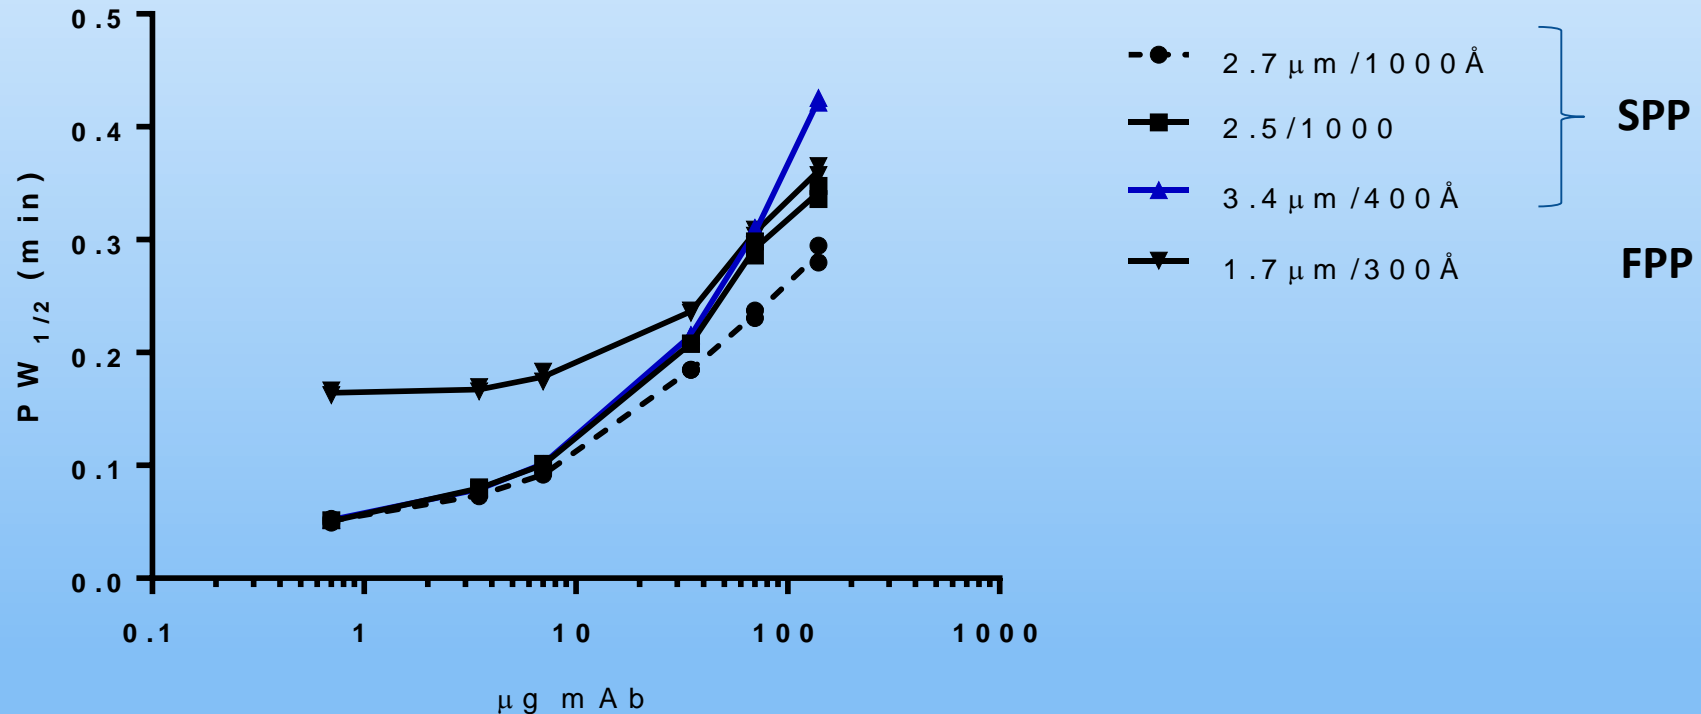


- For larger molecules, large pore SPP particles tolerate large sample masses effectively.
- Performance loss is progressive, occurring around 20-50 μg on column
- At all load levels 1000 \AA pore size SPP performed best for this mAb

Myosin LC/MS using 1000 Å Fused-Core Particles



Rabbit Skeletal Myosin Structure

2 HC subunits @ 220 kDa

4 LC subunits (2 x RLC @ 20 kDa + 2 ELC (17, 25 kDa))

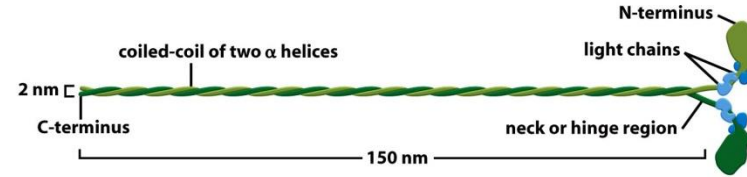

2.1 x 100 mm, 2.7 μm fused-core, C4, 1000 Å; 0.1% DFA 33 – 48% AcN in 50 min.;
Flow rate: 0.2 mL/min; Temp: 75°C; 2.5 μg myosin (7 M Urea/1% HOAc).

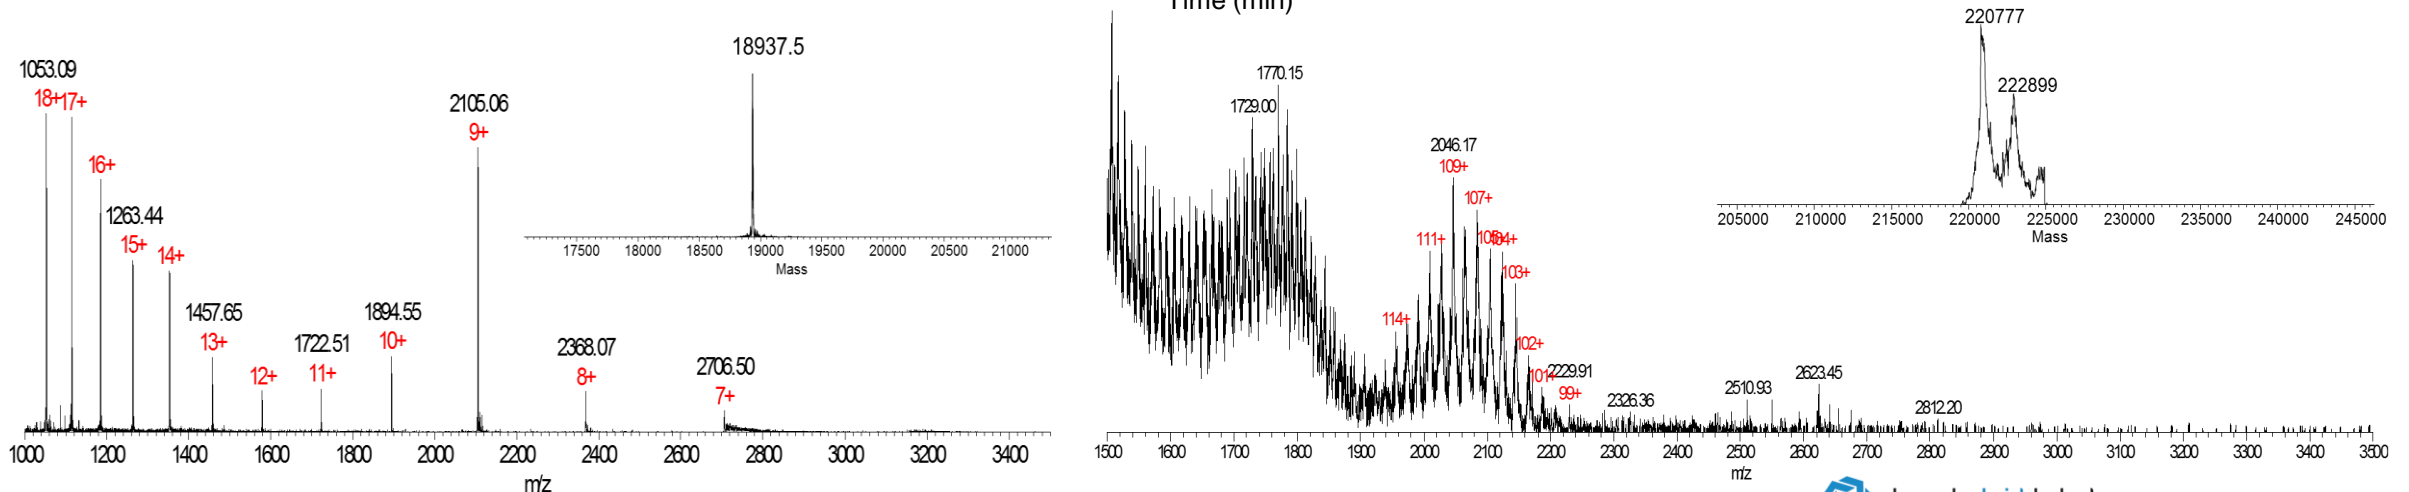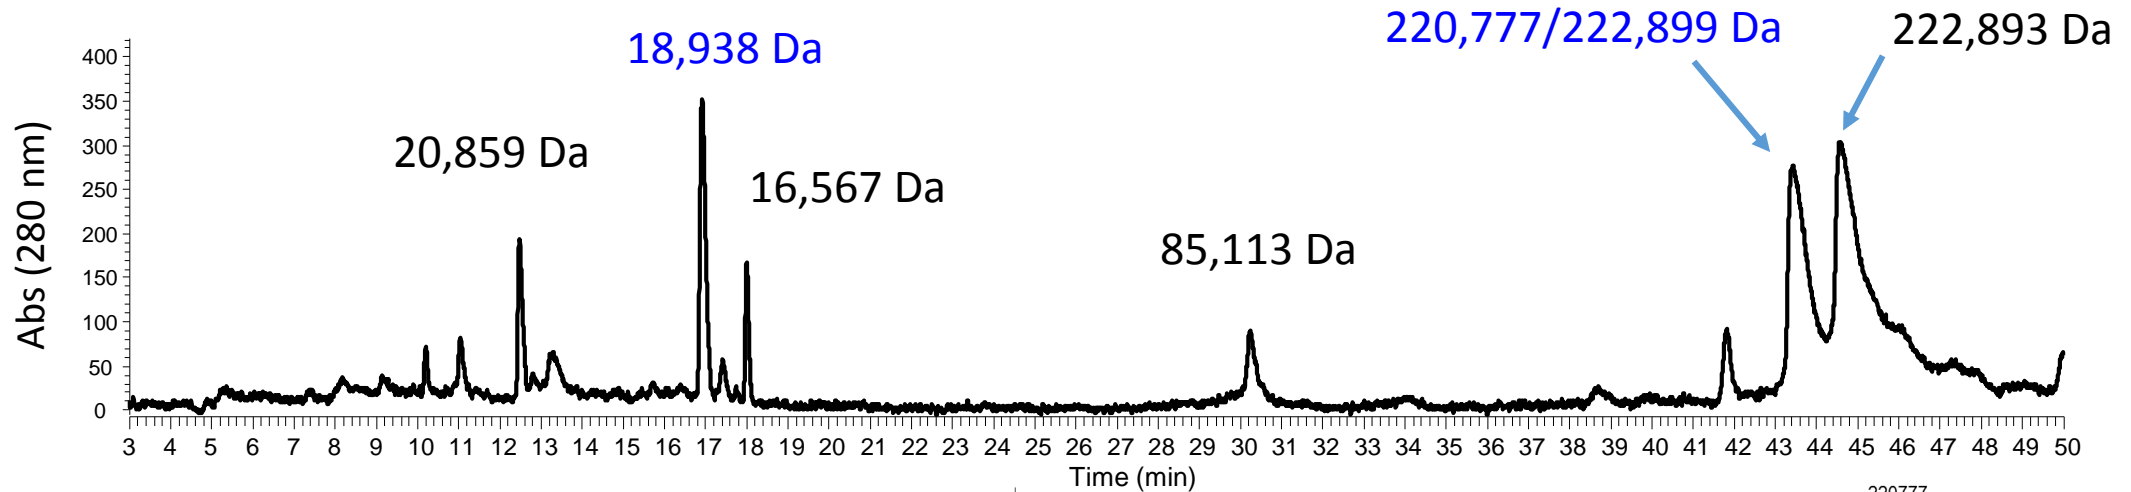

Adapted from Alberts, et al., *Molecular Biology of the Cell* (© Garland Science 2008)

Summary and Future Work

- Improving protein LC/MS is both materials and chemistry.
- DFA is current best practice in our labs, with more than 2 years of practical experience indicated no detrimental effects on MS or LC hardware. Exploring potential benefits of mixtures of DFA/FA, and examining benefit across flow rates.
- Restricted diffusion effects for proteins are demonstrated for IgGs and larger molecules, leading to effects on peak shape (widths) and load effects.
- Fused-Core with enlarged pore sizes (400 and 1000 Å) have particular utility for protein analyses, are highly robust, and allow *faster* protein separations with *higher* efficiency. Examining question of *if there is any disadvantage* to the use of largest feasible pores for generic protein separations.
- Continuing focus on the use of new materials (MP and SP) to enable larger biomolecule (>500 kDa) LC and LC/MS analysis.

Acknowledgements

Thank you for your Attention!

- AMT – Dr. Joe DeStefano, Mark Haynes, and Bob Moran.
- Proteomics and Glycoproteomics
 - Prof. Ron Orlando, U.Ga
 - D.J. Johnson, Shujuan Tao, Yining Huang, Emily Betchy and Majors Badgett, CCRC, University of GA.
- AMT and NIH/SBIR Program for Financial Support